

Pelvic C-Clamp

Emergency stabilization of sacrum fractures
or joint disruptions

Surgical Technique

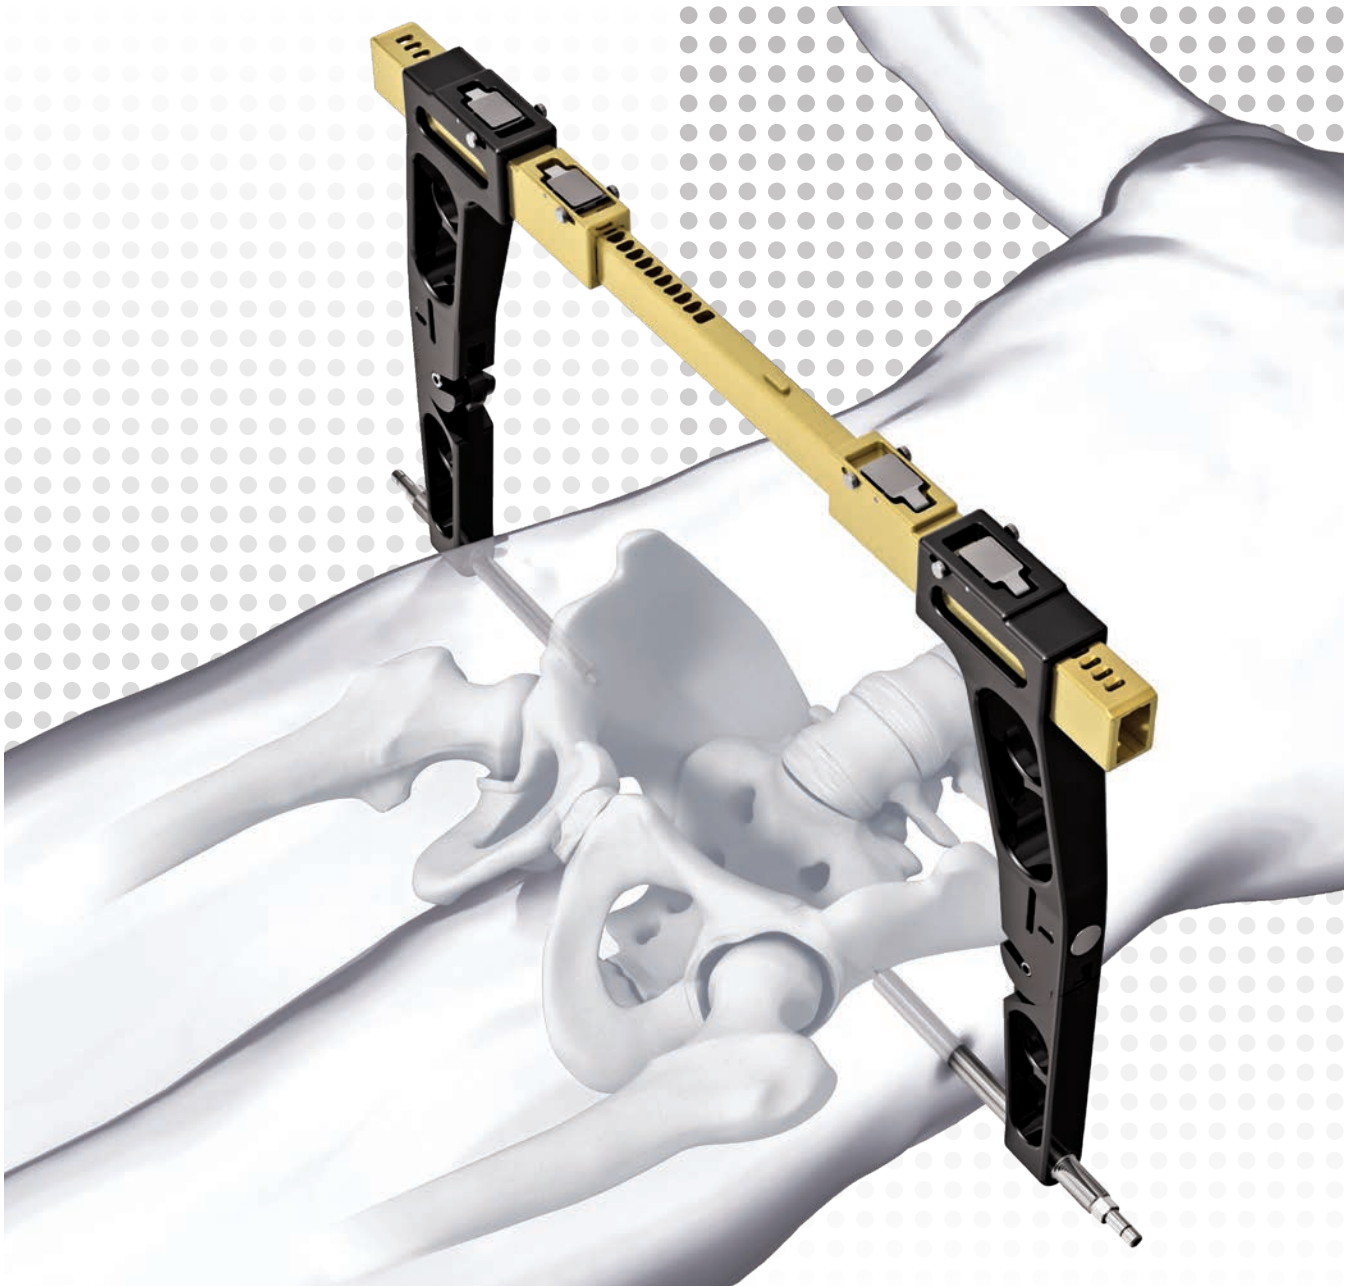


 Image intensifier control

This description alone does not provide sufficient background for direct use of DePuy Synthes products. Instruction by a surgeon experienced in handling these products is highly recommended.

Processing, Reprocessing, Care and Maintenance

For general guidelines, function control and dismantling of multi-part instruments, as well as processing guidelines for implants, please contact your local sales representative or refer to:

<http://emea.depuysynthes.com/hcp/reprocessing-care-maintenance>

For general information about reprocessing, care and maintenance of DePuy Synthes reusable devices, instrument trays and cases, as well as processing of DePuy Synthes non-sterile implants, please consult the Important Information leaflet (SE_023827) or refer to:

<http://emea.depuysynthes.com/hcp/reprocessing-care-maintenance>

Table of Contents

Introduction	Pelvic C-Clamp	2
	The AO Principles of Fracture Management	5

Surgical Technique		6
---------------------------	--	---

Disassembly and Maintenance		13
------------------------------------	--	----


Product Information	Implants and Instruments	15
	Set	16

MRI Information		17
------------------------	--	----

- Notes
- ▲ Precautions
- ▲ WARNINGS

Pelvic C-Clamp

Emergency stabilization of sacrum fractures or joint disruptions

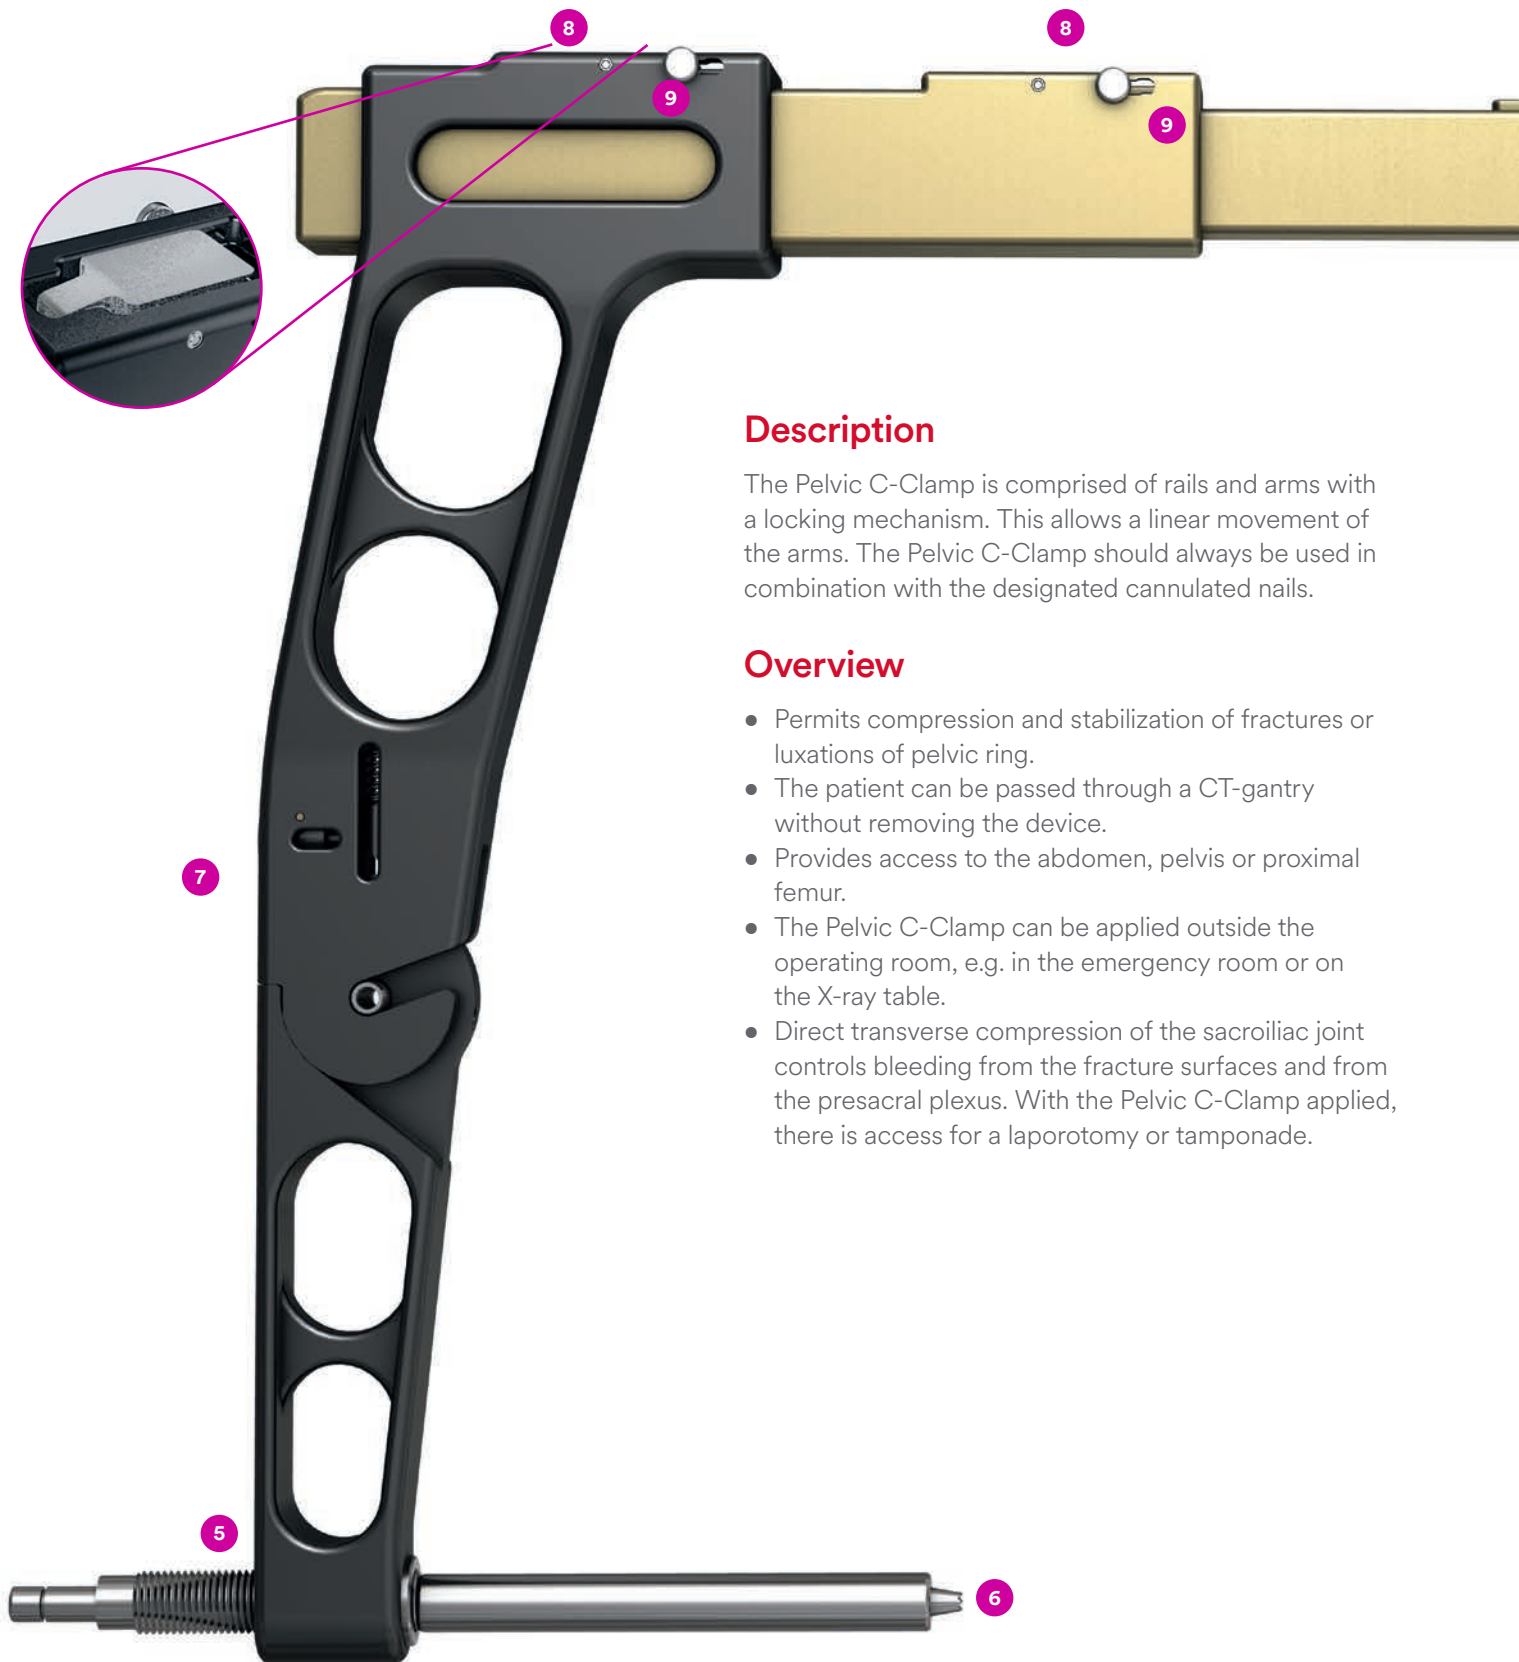


Description

The Pelvic C-Clamp is comprised of rails and arms with a locking mechanism. This allows a linear movement of the arms. The Pelvic C-Clamp should always be used in combination with the designated cannulated nails.

Overview

- Permits compression and stabilization of fractures or luxations of pelvic ring.
- The patient can be passed through a CT-gantry without removing the device.
- Provides access to the abdomen, pelvis or proximal femur.
- The Pelvic C-Clamp can be applied outside the operating room, e.g. in the emergency room or on the X-ray table.
- Direct transverse compression of the sacroiliac joint controls bleeding from the fracture surfaces and from the presacral plexus. With the Pelvic C-Clamp applied, there is access for a laparotomy or tamponade.

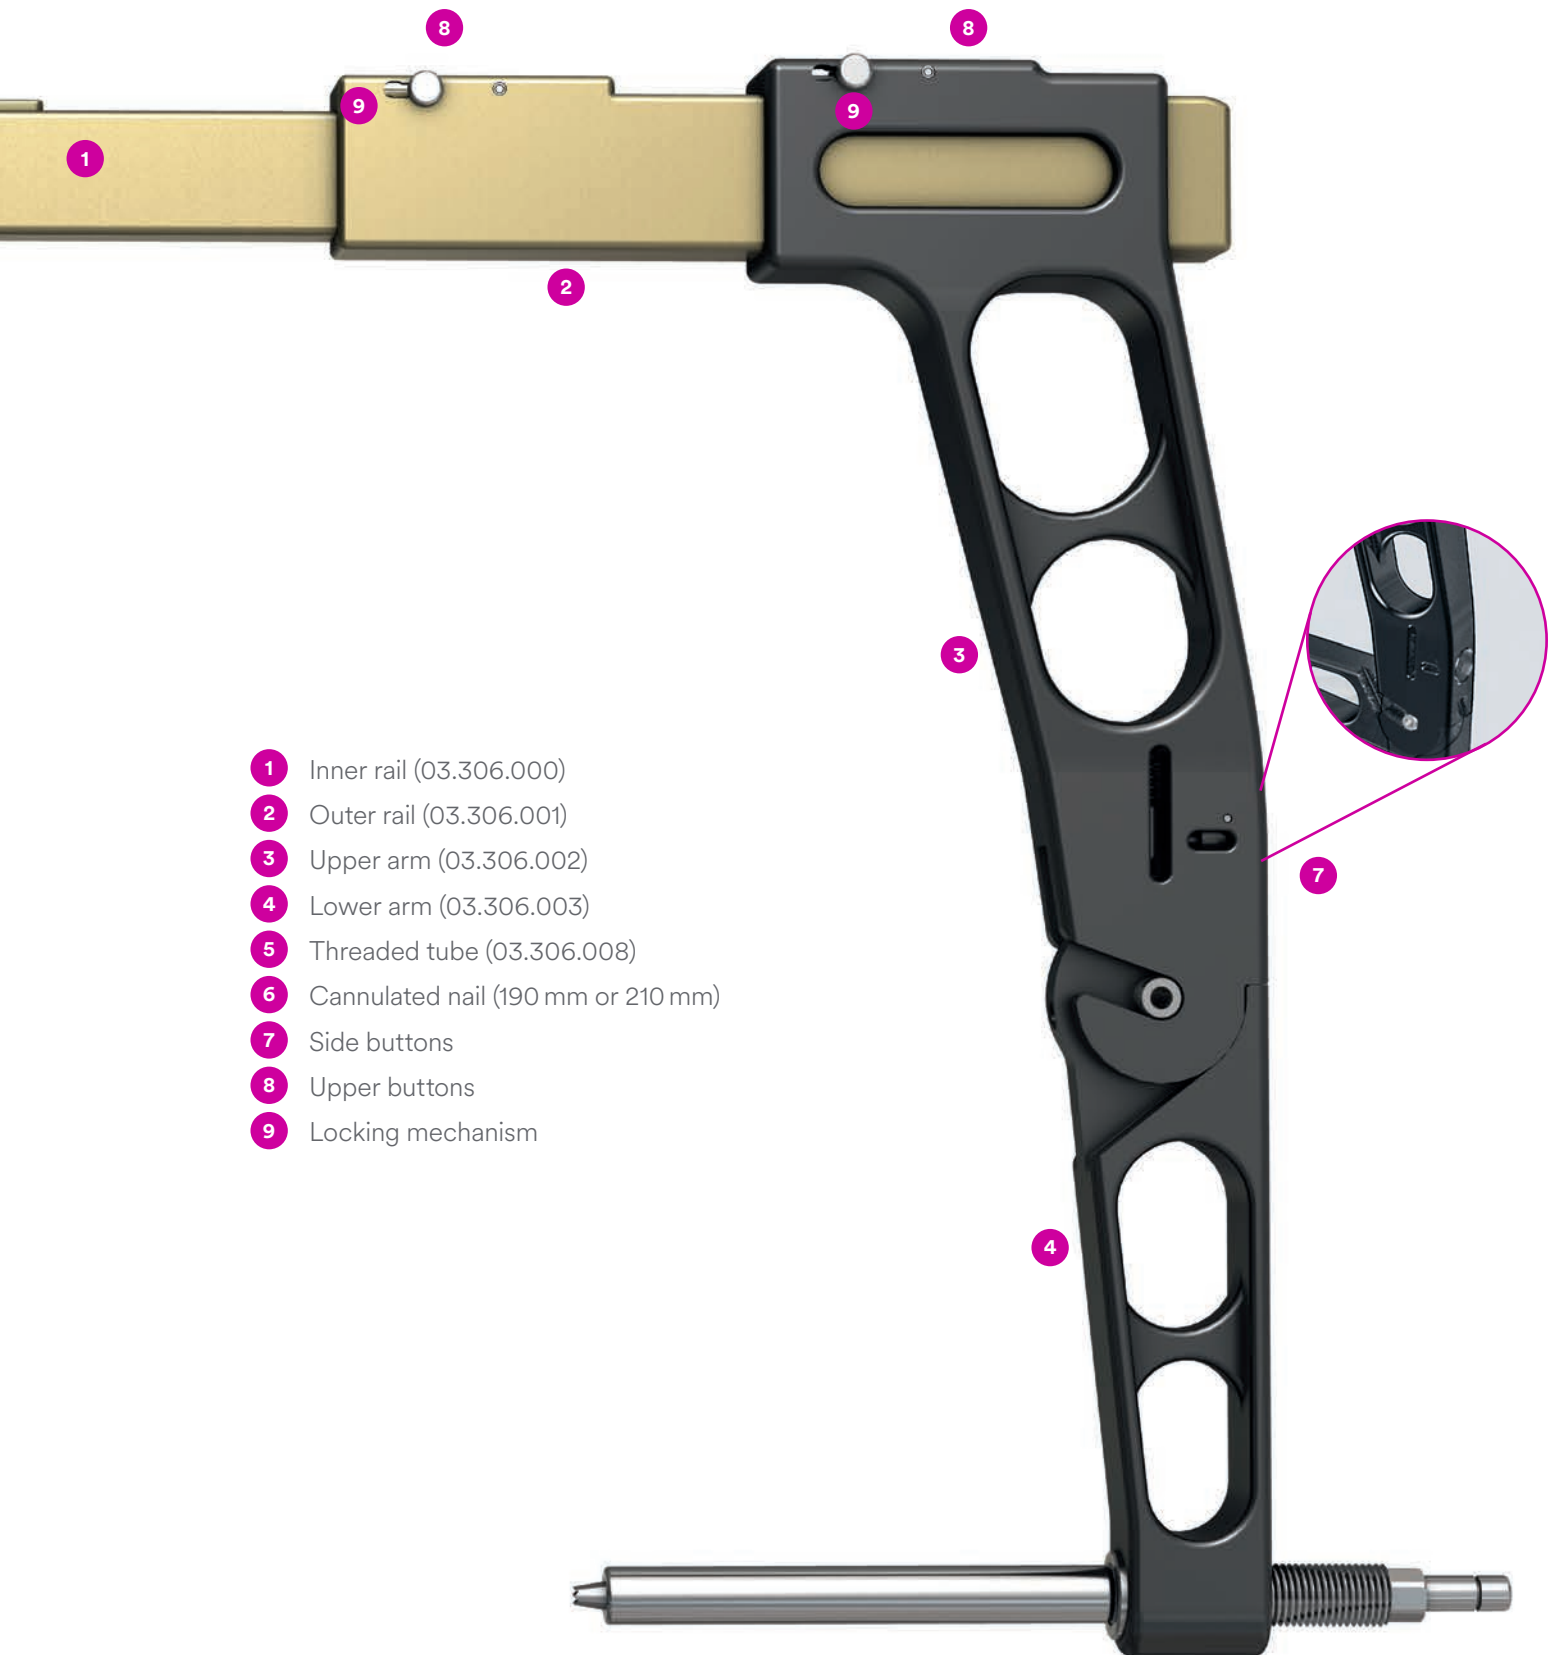

- 1 Inner rail (03.306.000)
- 2 Outer rail (03.306.001)
- 3 Upper arm (03.306.002)
- 4 Lower arm (03.306.003)
- 5 Threaded tube (03.306.008)
- 6 Cannulated nail (190 mm or 210 mm)
- 7 Side buttons
- 8 Upper buttons
- 9 Locking mechanism

▲ Precaution:

Avoid use where:

- Fractures of the ilium are present as there is risk of pin perforation through the fracture line
- There are comminuted sacral fractures with the risk of compression of the sacral nerve plexus

■ Note:

In life threatening situations hemorrhage control takes priority over the potential risk of nerve root compression.

Please refer to the corresponding instructions for use for specific information on intended use, indications, contraindications, warnings and precautions, Potential Adverse Events, Undesirable Side Effect and Residual Risks. Instruction for use are available at www.e-ifu.com and/or www.depuysynthes.com/ifu

The AO Principles of Fracture Management

Mission

The AO's mission is promoting excellence in patient care and outcomes in trauma and musculoskeletal disorders.


AO Principles^{1,2}

1.



Fracture reduction and fixation to restore anatomical relationships.

2.



Fracture fixation providing absolute or relative stability, as required by the “personality” of the fracture, the patient, and the injury.

3.



Preservation of the blood supply to soft-tissues and bone by gentle reduction techniques and careful handling.

4.



Early and safe mobilization and rehabilitation of the injured part and the patient as a whole.

¹ Müller ME, Allgöwer M, Schneider R, Willenegger H. Manual of Internal Fixation. 3rd ed. Berlin, Heidelberg New York: Springer 1991.

² Buckley RE, Moran CG, Apivatthakakul T. AO Principles of Fracture Management: 3rd ed. Vol. 1: Principles, Vol. 2: Specific fractures. Thieme; 2017.

Surgical Technique

1. Pre-operative preparation

Instrument

01.306.000 Pelvic C-Clamp complete set

The Pelvic C-Clamp set consists of the instruments and implants for the emergency treatment of the indicated fracture types. The bottom layer of the Vario Case houses the Pelvic C-Clamp and the optional pliers. The upper layer houses the cannulated nails in two lengths and the remaining instruments.

The complete sterile Pelvic C-Clamp set should be kept ready for use in the resuscitation room. Depending on the type of injury, the orientation points in the pelvic region of the injured person may be unclear. Should there be doubts about the anatomic references, use an image intensifier during application of the Pelvic-C-Clamp.

Pre-operative preparation

- Anteroposterior (AP) plain pelvic radiograph if necessary, oblique views (Inlet and Outlet) or CT.
- Patient positioning must allow for intraoperative fluoroscopic controls in AP, Inlet and Outlet Projections.
- Have an image intensifier available.

Positioning

- Place the patient in a supine position.
- To facilitate reduction, ensure free draping of the leg on the injured side. Strive for good draping coverage of the genital region.
- To prepare the patient, disinfect the proximal femur and the buttocks and cover with sterile sheets.

Preparation of the Pelvic C-Clamp

Open the lower side arms by depressing the buttons on the arms to prepare the Pelvic C-Clamp for use. (a)

■ Note:

Hold upper and lower arms with both hands and ensure that the lower arm is locked when fully extended.

Extend the upper bars by depressing the buttons on the upper rails while simultaneously pulling on the side arms. (b)

■ Note:





Maximal extension of the Pelvic C-Clamp is advantageous for easy positioning.

With a light twist, place the cannulated nails of preferred length into the threaded tubes. (c)

The teeth on the tip of the nail allow for grip onto the bone.

The buttons on the top of the Pelvic C-Clamp can be locked.

Ensure the buttons are not locked when applying the Pelvic C-Clamp to the patient, otherwise no or insufficient compression can be achieved.

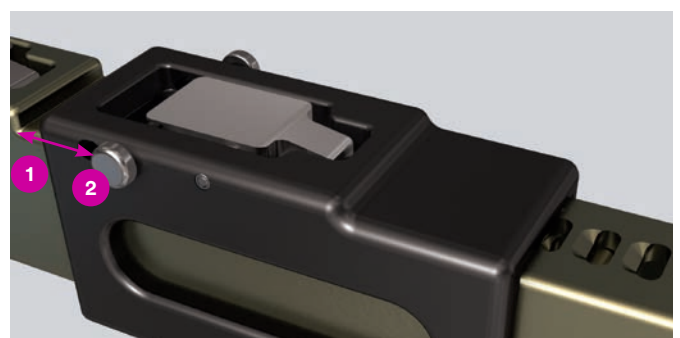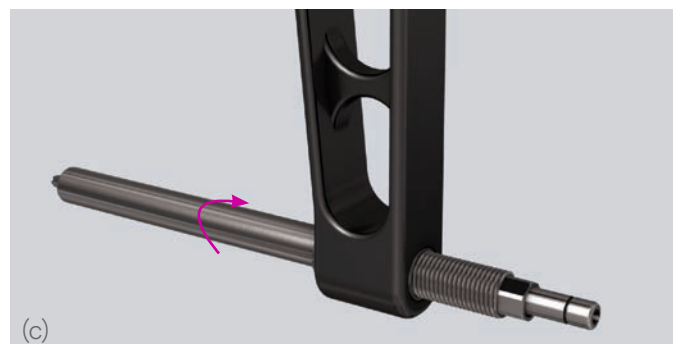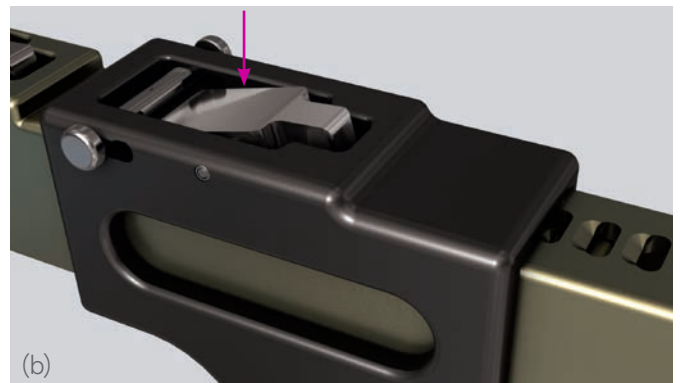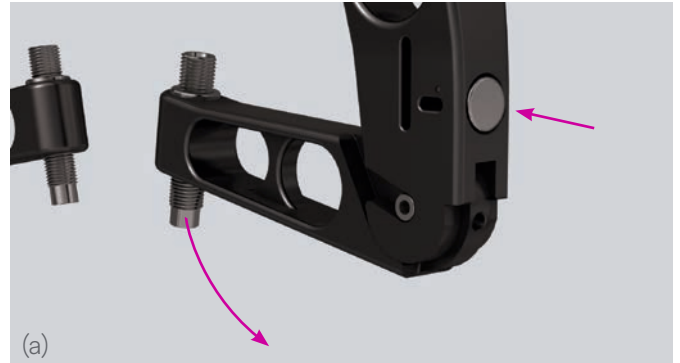

1 Unlock
2 Lock

2. Identifying nail insertion point

Instrument

03.306.009 Guide Handle, for Kirschner Wire
 Ø 2.5 mm



Make an incision at the intersection between the extension of the line of the femoral axis over the tip of the greater trochanter, and a vertical line from the anterior superior iliac spine in the dorsal direction (see illustration).

- If orientation is difficult, use an image intensifier.

The surface reference point of the outer side of the ilium changes at the level of the sacroiliac joints. In emergency situations, the resulting “fossa” can be used as a relatively secure point of reference aid. For secure anchoring, the Pelvic C-Clamp must be placed at the level of the sacroiliac joints.

▲ WARNINGS:

- If the nails are placed too ventrally to the correct insertion point, there is a risk of perforation of the ilium, which can result in organ injury.
- Placement of the pins in an excessively dorsal position may result in injury to gluteal nerves and vessels.
- Inserting the nail too distally endangers the sciatic nerve and the gluteal vessels in the sciatic notch. Malpositioning of the nail in osteoporotic bone, combined with excessive compression, can result in unwanted nail penetration.

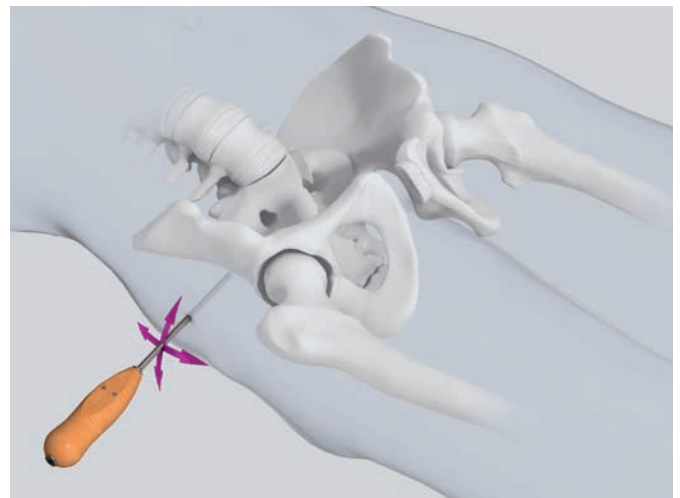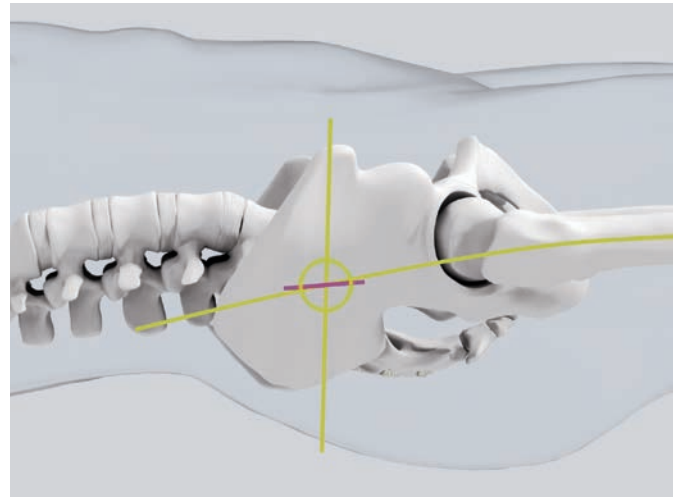

3. Kirschner Wire placement

Instruments

03.306.009	Guide Handle, for Kirschner Wire Ø 2.5 mm
292.260	Kirschner Wire Ø 2.5 mm with trocar tip, length 280 mm
398.320	Socket Wrench Ø 11mm with Hammer


After having identified the insertion point, a Kirschner Wire can be placed through the Guide Handle (only on the uninjured side). Gently hammer the Kirschner Wire into the bone with the Socket Wrench with Hammer. This Kirschner Wire will ensure an exact placement of the cannulated nail and prevents the nail from slipping.

■ Note:

Malpositioned Kirschner wires can be removed with the optional pliers.

▲ Precautions:

- Instruments and screws may have sharp edges or moving joints that may pinch or tear user's glove or skin.
- Handle devices with care and dispose worn bone cutting instruments in an approved sharps container.
- Select the appropriate Schanz screw for the patient's bony anatomy.

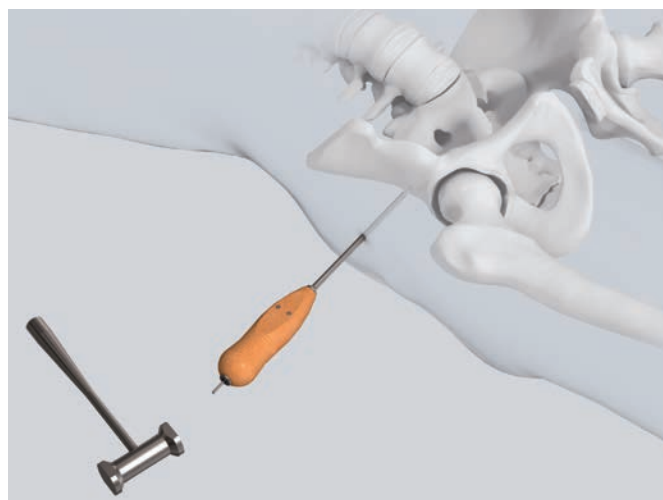

4. Placement of the Pelvic C-Clamp

Instruments

03.306.010	Pelvic C-Clamp, complete
02.306.006	Nail for Pelvic C-Clamp, cannulated, short, length 190 mm (2×)
or	
02.306.007	Nail for Pelvic C-Clamp, cannulated, long, length 210 mm (2×)
321.200	Ratchet Wrench for Nut, hexagonal, 11 mm

Optional instruments



359.204	Pliers, flat nosed
395.781	Cap

Be sure the fracture is correctly reduced before placement of the Pelvic C-Clamp.

After inserting the Kirschner Wire on the uninjured side, slide the clamp with cannulated nails over the wire and ensure that the tip of the nail grips the bone securely. Then place the second nail on the injured side (no Kirschner wire is necessary on this side).

■ Note:

In cases of severe dislocations of the pelvis, pulling on the leg, internal rotation and even lateral compression may improve reduction and facilitate application of the Pelvic C-Clamp.

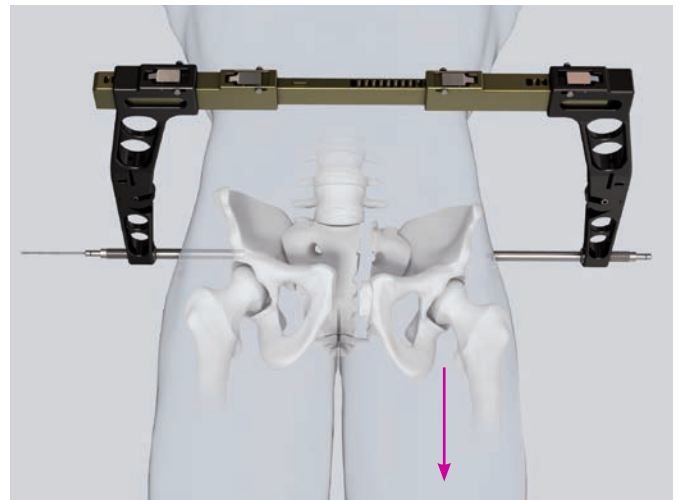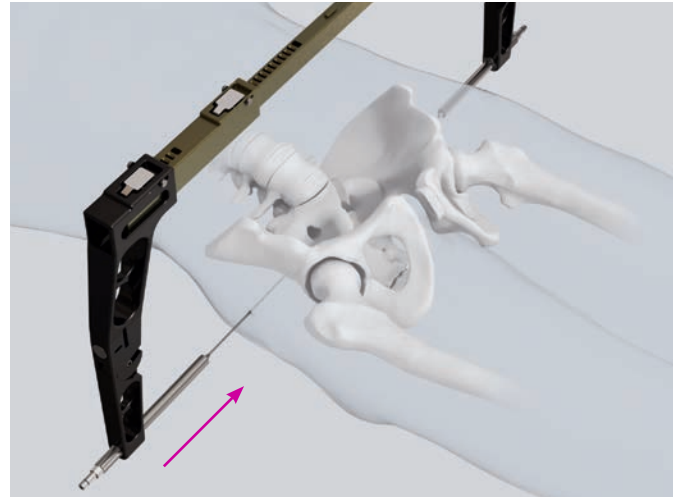

Alternative

Both nails can be placed at the same time. To do this take off one side arm. After both nails have been seated properly the arm can be placed over the rail again and compression can be achieved as described below.

When both nails are correctly seated, manually compress the upper side arms (a) and ensure final fixation by tightening the threaded tubes with the Ratchet Wrench (b).

The Kirschner wire must be removed with the wire cutter. If desired, place a protective cap on each end of the two cannulated nails.

- After complete application of the Pelvic C-Clamp, verify fixation with an image intensifier or X-ray (pelvic AP view) and pad the nails.

■ Note:

The locking mechanism locks the upper buttons, thus preventing unintended loss of compression during movement of the Pelvic C-Clamp.




Once mounted, the Pelvic C-Clamp can be swung caudally and cranially, e.g. for a laparotomy or an angiography.

■ Note:

It is recommended to place a drape cloth or lap sponges as a cushion between the Pelvic C-Clamp and the patient.

▲ WARNING:

Do not use the Pelvic C-Clamp to lift the patient.

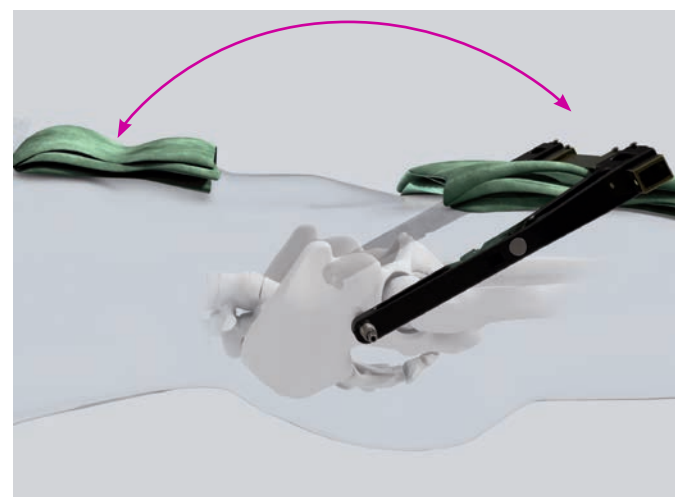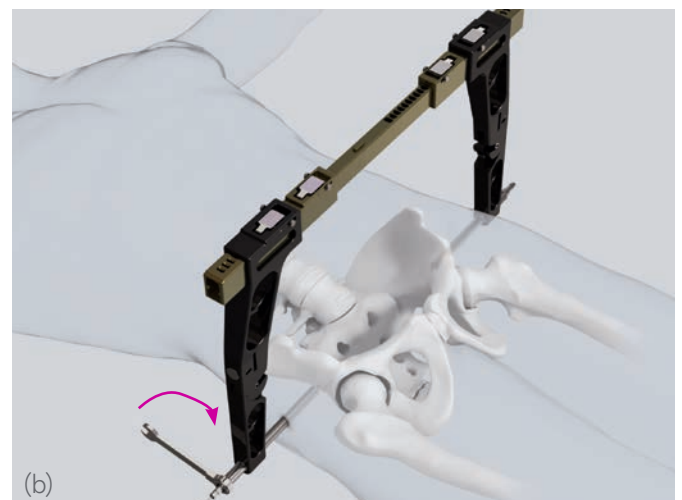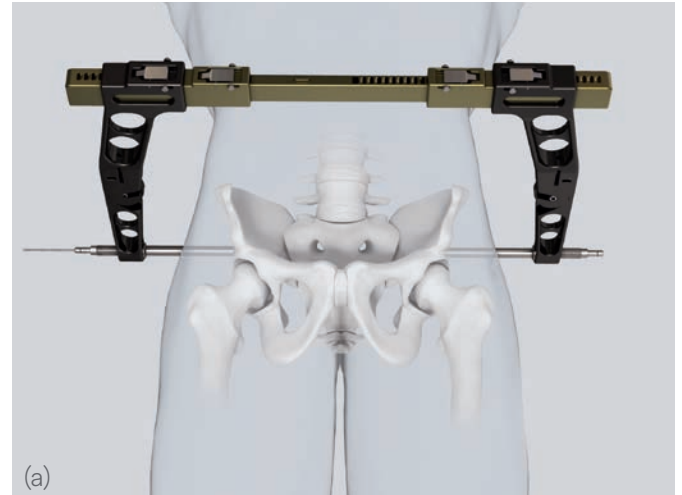

5. Postoperative management

- AP plain radiograph, CT if required, rarely oblique view films after application of Pelvic C-Clamp and during follow-up.
 - Do not use the Pelvic C-Clamp to lift the patient.
 - Wound closure; extended incisions may require a coapting skin suture.
 - Continuing injury management according to polytrauma protocols.
 - The nail insertion sites must be meticulously disinfected and dressed.
 - Avoid turning the patient sideways as this could cause one of the nails to penetrate the bone excessively.
-

6. Removal


The Pelvic C-Clamp must be removed prior to definitive treatment of the posterior pelvic ring injury. Be sure to remove protective caps from cannulated nails and Kirschner wire from uninjured side.

Disassembly of the Pelvic C-Clamp


Note:

Before cleaning, the Pelvic C-clamp should be disassembled.


The lower arms can be raised (2) by pressing the side buttons (1) as depicted by the red arrows.

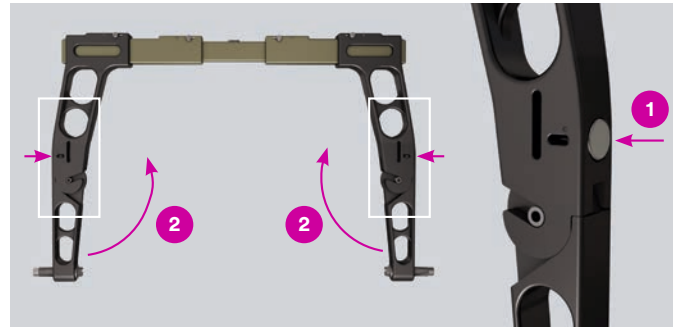


To remove the lower arms completely, keep pushing the buttons (1) and slide the arms out (2).

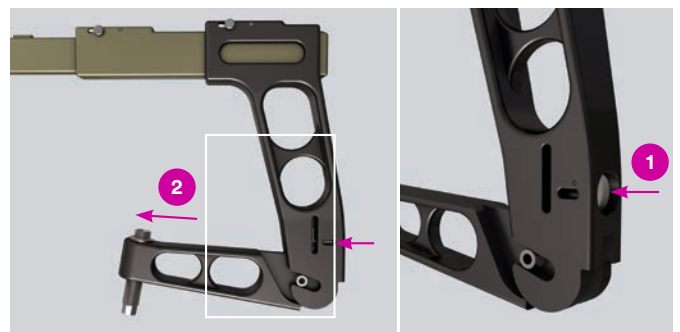


Unscrew the threaded tubes from the lower arms.

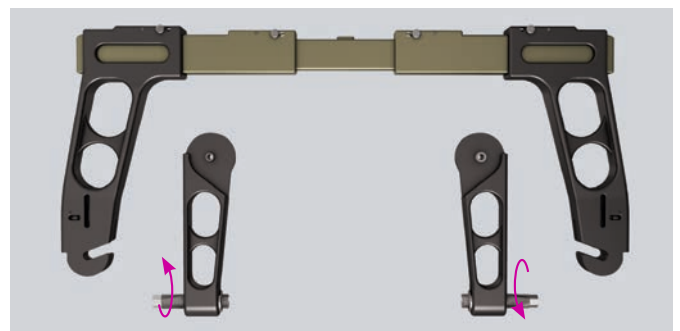


Before removing the upper arms from the upper rails, make sure the locking mechanism is unlocked (1). The upper arms can then be removed by pressing the top buttons (2) while simultaneously pulling on the arms (3). Be sure to hold the rails during this procedure to prevent the rails from falling.

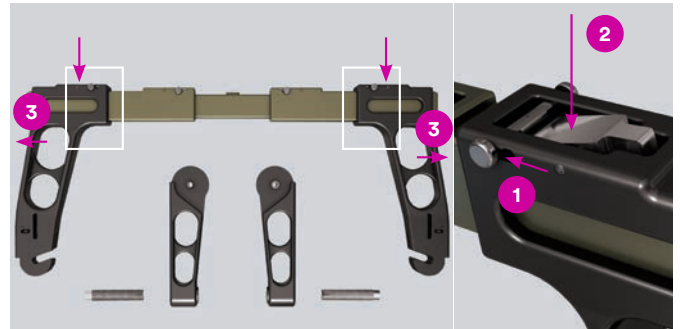

The outer rails can be separated from the inner rail by pressing the buttons on the outer rails and pulling the two rails apart (3).

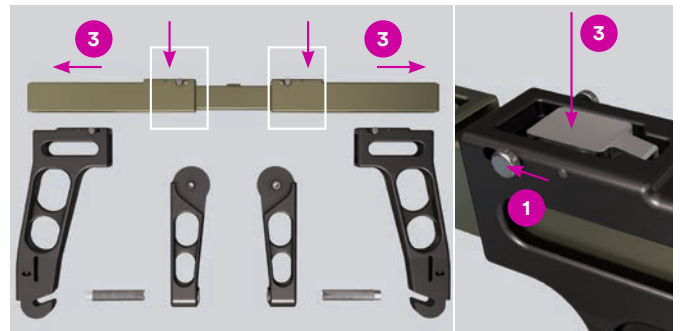

After disassembly, clean the rails, arms and threaded tubes manually, e.g. by using a brush. The springs in the upper arm at button should be cleaned too. If necessary, broken or damaged parts should be exchanged.

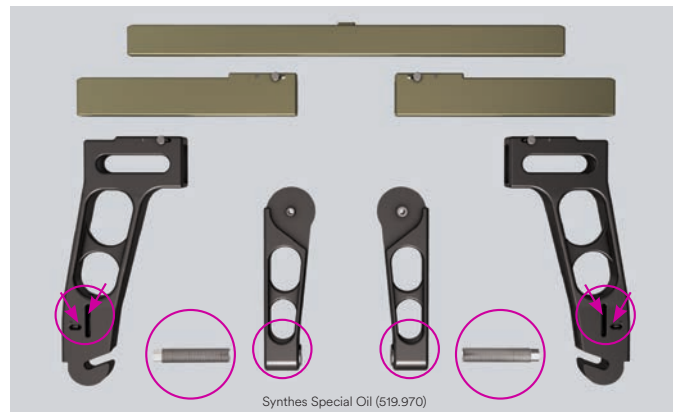

After cleaning, oil the thread of the threaded tube as well as the two holes next to the side buttons with DePuy Synthes special oil (see red circles) and reassemble the device.

The Pelvic C-Clamp should be checked after every use/cleaning/sterilization to confirm correct function, i.e. that all parts move freely as intended.

The complete sterile Pelvic C-Clamp should be kept ready for use in the resuscitation room.

Due to the fact that the Pelvic C-Clamp consists of stainless steel, aluminum and a few pieces of polymer, it should only be cleaned at temperatures below 140°C and at a pH level between 7 and 9.5 (detergents).

Note:

The cannulated nails are only for single use.

Implants and Instruments

02.306.006 Nail for Pelvic C-Clamp, cannulated, short, length 190 mm



02.306.007 Nail for Pelvic C-Clamp, cannulated, long, length 210 mm



292.260 Kirschner Wire Ø 2.5 mm with trocar tip, length 280 mm



03.306.009 Guide Handle, for Kirschner Wire Ø 2.5 mm



321.200 Ratchet Wrench for Nut, hexagonal, 11 mm



398.320 Socket Wrench Ø 11 mm with Hammer



359.204 Pliers, flat-nosed



395.781 Cap



Set

Pelvic C-Clamp Set

01.306.000	Pelvic C-Clamp complete set
------------	-----------------------------

This set contains:

68.306.000	Vario Case for Pelvic C-Clamp, no contents	1
03.306.010	Pelvic C-Clamp (assembled, complete without nails)	1
02.306.006	Nail for Pelvic C-Clamp, cannulated, short, length 190 mm	2
02.306.007	Nail for Pelvic C-Clamp, cannulated, long, length 210 mm	2
321.200	Ratchet Wrench for Nut, hexagonal, 11 mm	2
398.320	Socket Wrench Ø 11 mm with Hammer	1
03.306.009	Guide Handle, for Kirschner Wire Ø 2.5 mm	1
292.260	Kirschner Wire Ø 2.5 mm with trocar tip, length 280 mm	10

The Pelvic C-Clamp (03.306.010) is comprised of the following articles that can be ordered separately as replacement parts:

03.306.000	Inner Rail for Pelvic C-Clamp	(1)
03.306.001	Outer Rail for Pelvic C-Clamp	(2)
03.306.002	Upper Side Arm for Pelvic C-Clamp	(2)
03.306.003	Lower Side Arm for Pelvic C-Clamp	(2)
03.306.008	Threaded Tube for Pelvic C-Clamp	(2)

Also available:

519.970	Special Autoclavable Oil
689.886	Container, extra-small, closable, without Contents, to accommodate Art. No. 395.781

Optional instruments:

359.204	Pliers, flat nosed
395.781	Cap

MRI Information

The “Pelvic C Clamp” is MR unsafe. Do not use this device in any MR environment. This device is known to pose hazards in all MR environments.

Please refer to the corresponding Instructions for Use for specific information on Intended use, Indications, Contraindications, Warnings and Precautions, Potential Adverse Events, Undesirable Side Effect and Residual Risks. Instruction for Use are available at www.e-ifu.com and/or www.depuysynthes.com/ifu

Not all products are currently available in all markets.
This publication is not intended for distribution in the USA.



Synthes GmbH
Eimattstrasse 3
4436 Oberdorf
Switzerland
Tel: +41 61 965 61 11

www.depuysynthes.com